



Performance Evaluation of PATHFAST Instrument & Reagents of Mitsubishi Chemical Europe

Evaluation Site: Sweden

Monica Vikner

Centralsjukhuset i Karlstad
Klin kem lab
65185 Karlstad

Correlation for cTnI: PATHFAST and Abbott Architect

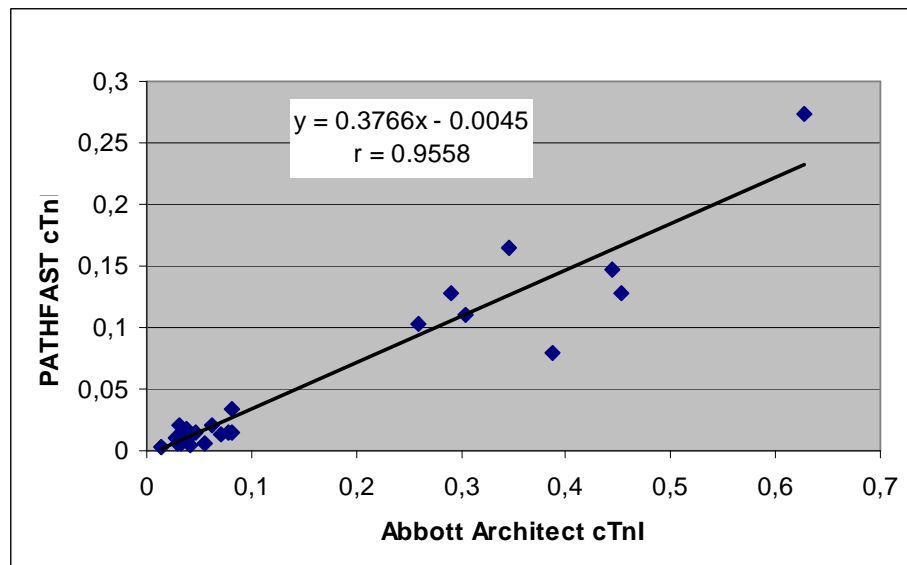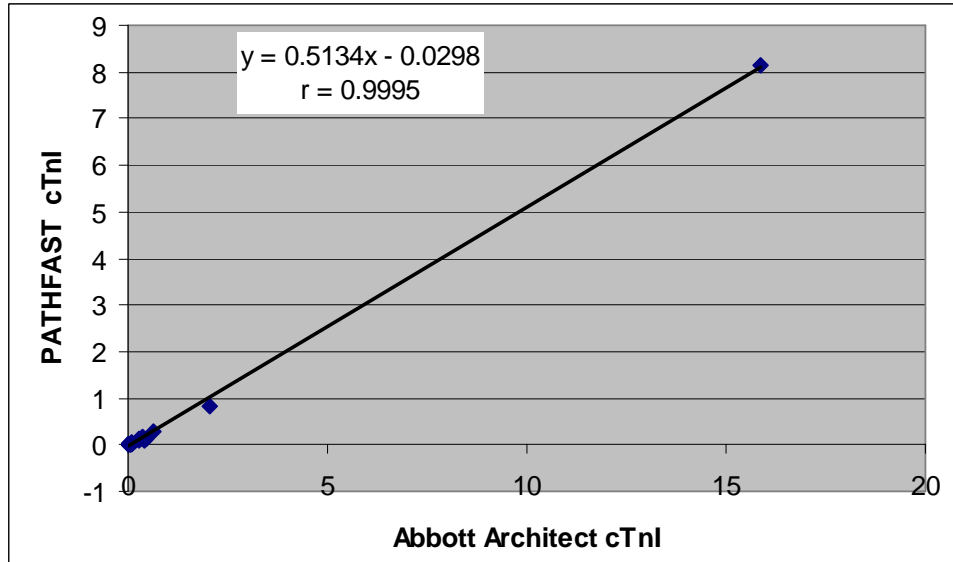

PATHFAST Cardiac Troponin I

Analytical sensitivity: 0.02 µg/L

99th percentile: <0.02 µg/L

Interferences:

Hemolysis – hemoglobin at 10 g/L <10%

Lipemia – Triglycerides at 11.3 mmol/L <10%